


PULSE GENERATOR PERFORMANCE

CHECK

Model: AVI

S.N.: 214

Date: MAY 30 '79

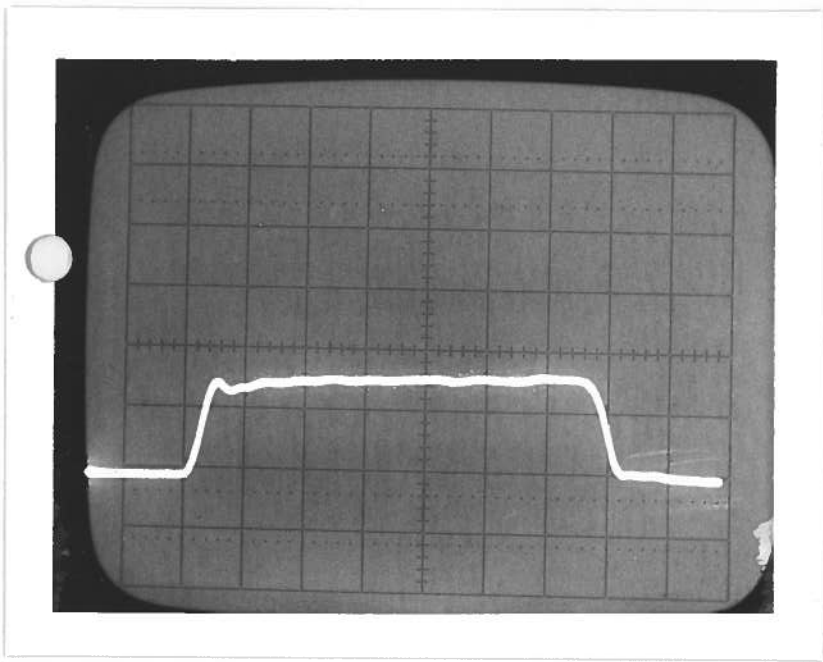

1.0 nsec/div
10 volts/div

- a) Output signal amplitude: *
15 VOLTS.
- b) Pulse width:
1.0 TO 100 nsec
- c) Rise time:
300 psec
(10% RISE TIME)
- d) Fall time:
< 1.0 nsec.
- e) PRF:
OK (SEE FILE 2)
- f) Jitter, stability:
OK
- g) Prime power:
+15 ± 1 VOLT
160 mA

* INTERNAL ATTENUATOR
INSTALLED IN AVI
S.N. 214 TO REDUCE
OUTPUT FROM 40 V TO
15 VOLTS.