


PULSE GENERATOR
PERFORMANCE CHECK

Model: AVO-2L-B-PN

S.N.: 9904

Date: Aug 31, 2001

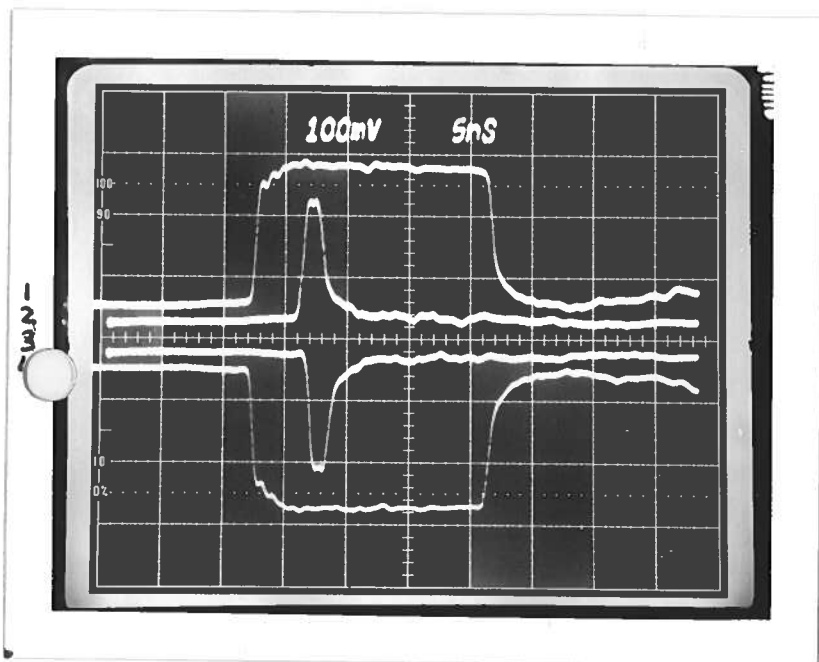

- a) Output signal amplitude:
0 to $\pm 25V$, into 12.5Ω
- b) Pulse width: 2-20ns
- c) Rise time: $\leq 0.5ns$
- d) Fall time: $\leq 0.5ns$
- e) PRF: 1Hz - 20kHz
- f) Jitter, stability: OK
- g) Prime power: 120/240V
50-60Hz

11V/div, 5ns/div, $R_L = 12.5\Omega$

- 1) +25V, 20ns PW
- 2) +25V, 2ns PW
- 3) -25V, 2ns PW
- 4) -25V, 20ns PW

Measured with AVX-BP-1
high impedance scope probe.



AVTECH ELECTROSYSTEMS LTD.

NANOSECOND WAVEFORM ELECTRONICS
SINCE 1975

P.O. BOX 265
OGDENSBURG, NY
U.S.A. 13669-0265
TEL: (315) 472-5270
FAX: (613) 226-2802

TEL: 1-800-265-6681
FAX: 1-800-561-1970

e-mail: info@avtechpulse.com
http://www.avtechpulse.com

P.O. BOX 5120 STN. F
OTTAWA, ONTARIO
CANADA K2C 3H4
TEL: (613) 226-5772
FAX: (613) 226-2802

"-B" Functional Test & Calibration Certificate

Date of test:	August 31, 2001				Tester:	MJC
Programmed model name:	AVO-2L-B-PN					
Programmed serial number:	9904					
Firmware revision:	2.27					
Internal trigger checked at:	2 Hz	20 Hz	200 Hz	2 kHz	20 kHz	
Actual measured output ¹ :	2.01 Hz	20.05 Hz	200.3 Hz	2.01 kHz	19.96 kHz	
External trigger checked:	yes			Gate checked:	yes	
Manual trigger checked:	yes					
Pulse compression checked:	yes		Low Amplitude PW Distortion Nulled:		N/A	
Pulse width checked at:	2 ns	5 ns	10 ns	20 ns	10 kHz, +20V, mainframe out	
Actual measured output ² :	2.1 ns	4.8 ns	9.7 ns	19.8 ns		
PW _{in} = PW _{out} mode checked:	N/A			DC mode checked:	N/A	
Duty Cycle Limit:	N/A					
Delay nulled:	yes					
Delay checked at:	100 ns	200 ns	500 ns		10 kHz, +20V, mainframe out	
Actual measured output ¹ :	99.6 ns	200.5 ns	505 ns			
Double pulse checked:	N/A					
Invert mode checked:	N/A					
ECL/TTL modes checked:	N/A					
Zout switch checked:	N/A					
Amplitude checked at:	-5V	+10V	-20V	+25V	10 kHz, +25V, to 12.5 Ohms	
Actual measured output ² :	-4.8V	+9.7V	-19.7V	+25.0V		
Amplitude polarity:	+/-					
Zout calibration:	N/A					
Electronic amplitude control:	N/A					
External amplify mode:	N/A					
Ultravolt flux removed:	N/A					
Monitor V/I Ratio:	N/A			Monitor offset nulled:		
LCD Monitor calibrated:	N/A			Monitor offset nulled:		
Offset checked at:	N/A					
Actual measured output ² :	N/A					
Offset nulled (output on):	N/A			Amplitude-dependent offset nulled:		
Offset nulled (output off):	N/A					
RS-232 checked:	yes					
Sync pulse width checked:	200 ns					
Circuit Boards:	PS:	93	Main:	108B		
Overload Trigger Resistance:	Trips at:	N/A	Installed:	N/A		
DC fuses:	Positive:	1A	Negative:	N/A		
AC Current at 115 VAC:	Quiescent:	0.40A	Max. Load:	0.41A		
AC fuse:	1A					
Photographed:	yes					

¹ Checked with: Fluke PM6681 Counter, referenced to Datum ExacTime 9390-6000 GPS Frequency Reference

² Checked with: Tektronix TDS3052 digital oscilloscope for PW ≥ 5 ns,
Tektronix 7704A/7S11/7T11/S4 sampling oscilloscope system for PW < 5 ns.