



AVTECH ELECTROSYSTEMS LTD.

NANOSECOND WAVEFORM ELECTRONICS
SINCE 1975

P. O. BOX 265
OGDENSBURG, NY
U.S.A. 13669-0265
TEL: (315) 472-5270
FAX: (613) 226-2802

TEL: 1-800-265-6681
FAX: 1-800-561-1970


e-mail: info@avtechpulse.com
<http://www.avtechpulse.com>

P.O. BOX 5120 STN. F
OTTAWA, ONTARIO
CANADA K2C 3H4
TEL: (613) 226-5772
FAX: (613) 226-2802

INSTRUCTIONS

MODEL AVX-BP-2

The AVX-BP-2 should be tested in the basic fashion shown below. Note that either connector of the probe may serve as the input. Also note that when displaying fast rise time waveforms the input to the probe should be shunted by a fifty ohm termination and the length of line between the termination and the probe input should be as short as possible (eg. 1 cm).

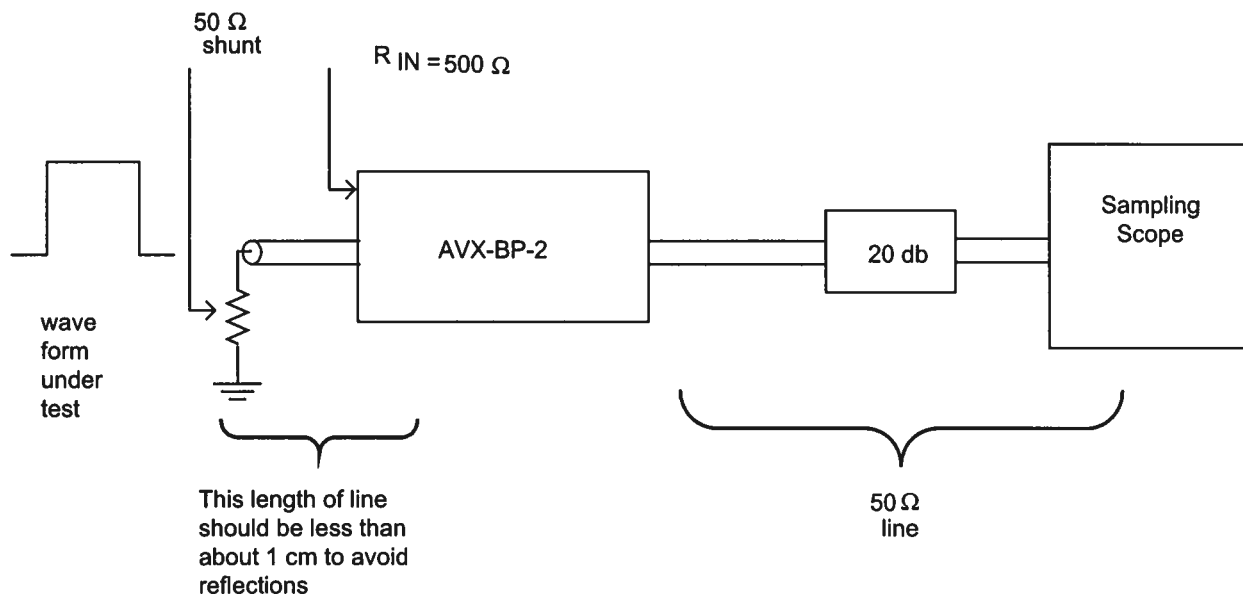



AVTECH ELECTROSYSTEMS LTD.

NANOSECOND WAVEFORM ELECTRONICS
SINCE 1975

P.O. BOX 265
OGDENSBURG, NY
U.S.A. 13669-0265
TEL: (315) 472-5270
FAX: (613) 226-2802

TEL: 1-800-265-6681
FAX: 1-800-561-1970


e-mail: info@avtechpulse.com
<http://www.avtechpulse.com>

P.O. BOX 5120 STN. F
OTTAWA, ONTARIO
CANADA K2C 3H4
TEL: (613) 226-5772
FAX: (613) 226-2802

INSTRUCTIONS

MODEL AVX-BP-2

The AVX-BP-2 should be tested in the basic fashion shown below. Note that either connector of the probe may serve as the input. Also note that when displaying fast rise time waveforms the input to the probe should be shunted by a fifty ohm termination and the length of line between the termination and the probe input should be as short as possible (eg. 1 cm).

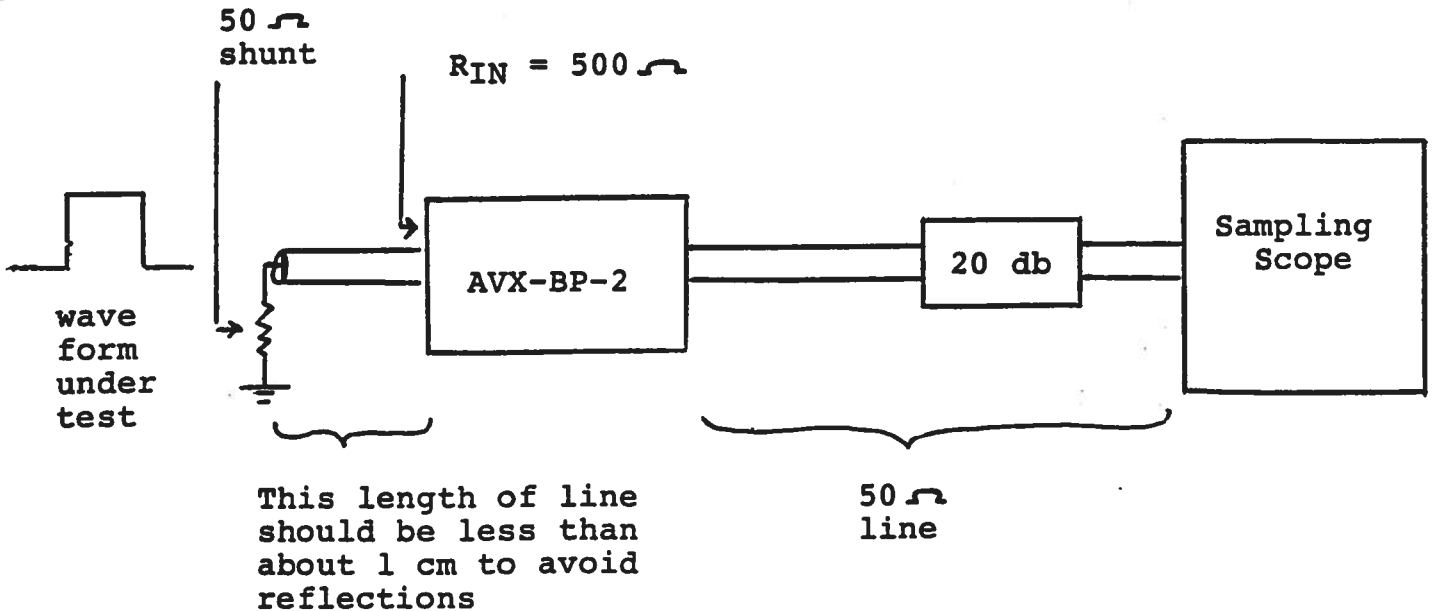

Oct 24 / 02